


# No electric power required at all!

**Repetitive Pipette** 



## Aspirate the sample all at once, dispensing its necessary volume repetitively.

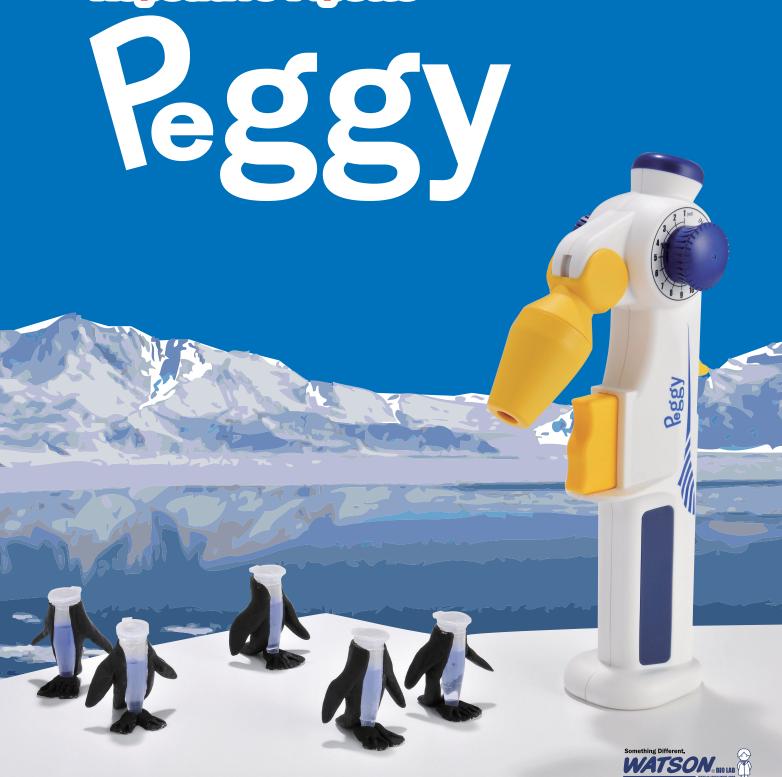

Dispensing button


Push in the aspiration button once slowly until the end to aspirate the set volume.

A single push of the dispensing button dispensed the set volume.


Can also change the dispensing capacity Note once per minute.

## Setting aspiration volume

### Setting dispensing volume



1mL1mL1mL1mL



Dispensing can be set in every 0.5mL for setting range 0.5 -5mL.



Adjustable nozzle angle in every 10 degrees up 50 degrees.

### Simple maintenance



Easy to remove & set spare parts

- Nozzle cover: Autoclavable
- Joint packing: Autoclavable

- water	stop iliter: R	epiaceable

Cat.No.	Item	Aspiration Volume max. min.	Discharge Volume max. min.	Packaging
PG-01	PEGGY-01 Repetitive Pipette "Peggy"	13 mL 1 mL	5 mL 0.5 mL	1 unit / box

### Precaution in case of using 5mL serological pipette:

Please DO NOT set aspiration volume exceeding 5mL in case that 5mL serological pipette is used. It may cause an accidental liquid suction leading to malfunction on Peggy.

1mL for setting range 1-13mL.

Note: 13mL can be dispensed in case that Watson 10mL Serological Pipette is used.



Manufactured and sold by:

FUKAEKASEI CO., LTD.

Head Office: 2-2-7 Murotani, Nishi-ku, Kobe

651-2241 JAPAN TFI +81-78-991-4477 FAX +81-78-991-4491

E-mail: info@watson.co.jp https://watsonbiolab.com

